



AssayMax Mouse Insulin-like Growth Factor 1 (IGF-1) ELISA Kit

Catalog # EMI1001-1

Introduction

Insulin-like growth factor 1 (IGF-1) is a 70 amino acid polypeptide protein hormone with molecular mass of 7.65 kDa (1). IGF-1 is produced primarily by the liver in response to the stimulation of growth hormone. It is transported in plasma bound to different forms of IGF-1 binding proteins (2). It also binds to specific IGF-1 tyrosine kinase receptor and the insulin receptor. Inhibition IFG-1 receptor reduces pancreatic cancer growth and angiogenesis (3). IGF-I regulates cellular proliferation, differentiation, apoptosis, and amyloid precursor protein family (4 - 5). It may be important in the pathophysiological processes underlying chronic disease, including type 2 diabetes mellitus, coronary heart disease, cancer and Alzheimer's disease (6 - 8). Increased levels of IGF lead to an increased risk of cancer (9). IGF-I stimulates osteoblast proliferation, bone formation, and increases bone volume (10). It is a potent neurotrophic as well as a neuroprotective factor found in the central and the peripheral nervous systems of the brain (11).

Principal of the Assay

The AssayMax Mouse IGF-1 ELISA kit is designed for detection of mouse IGF-1 in plasma, serum and cell culture supernatants. This assay employs a quantitative sandwich enzyme immunoassay technique, which measures IGF-1 in 5 hours. A polyclonal antibody specific for mouse IGF-1 has been pre-coated onto a microplate. Mouse IGF-1 in standards and samples is sandwiched by the immobilized antibody and biotinylated polyclonal antibody specific for mouse IGF-1, which is recognized by a streptavidin-peroxidase conjugate. All unbound material is then washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured.

Caution and Warning

- This kit is for research use only.
- The kit should not be used beyond the expiration date.
- The Stop Solution is an acid solution.

Reagents

- **Mouse IGF-1 Microplate:** A 96 well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody against mouse IGF-1.
- **Sealing Tapes:** Each kit contains 3 pre-cut, pressure-sensitive sealing tapes, which can be cut to fit the format of the individual assay.
- **Mouse IGF-1 Standard:** Recombinant mouse IGF-1 in a buffered protein base (10 ng, lyophilized).

- **Biotinylated IGF-1 Antibody (100x):** A 100-fold concentrated biotinylated polyclonal antibody against IGF-1 (80 µl).
- **Streptavidin-Peroxidase Conjugate (SP Conjugate):** A 100-fold concentrate (90 µl).
- **MIX Diluent Concentrate (10x):** A 10-fold concentrated buffered protein base (30 ml).
- **Wash Buffer Concentrate (20x):** A 20-fold concentrated buffered surfactant (30 ml).
- **Chromogen Substrate:** A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution:** A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

Storage Condition

- Store unopened kit at 2 - 8⁰C up to expiration date.
- Opened MIX Diluent may be stored for up to 1 month at 2 - 8⁰C. Store reconstituted reagents at <-20⁰C.
- Opened unused strip wells may return to the foil pouch with the desiccant pack, reseal along zip-seal. May be stored for up to 1 month in a vacuum desiccator.

Other Supplies Required

- Microplate reader capable of measuring absorbance at 450 nm.
- Pipettes (1-20 µl, 20-200 µl, 200-1000 µl and multiple channel).
- Deionized or distilled reagent grade water.

Sample Collection and Storage

- **Plasma:** Collect plasma using one-tenth volume of 0.1 M sodium citrate as an anticoagulant. Centrifuge samples at 2000 x g for 10 minutes and assay. Dilute samples 1:250 into MIX Diluent. Store samples at -20⁰C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Serum:** Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 2000 x g for 10 minutes. Remove serum and assay. Dilute samples 1:250 into MIX Diluent. Store serum at -20⁰C or below. Avoid repeated freeze-thaw cycles.
- **Cell Culture Supernatants:** Centrifuge cell culture media at 2000 x g for 10 minutes to remove debris. Collect supernatants and assay. Store samples at -20⁰C or below. Avoid repeated freeze-thaw cycles.

Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use. If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved.
- **MIX Diluent Concentrate (10x):** Dilute the MIX Diluent Concentrate 1:10 with reagent grade water. Store for up to 1 month at 2 - 8⁰C.
- **IGF-1 Standard:** Reconstitute the 10 ng of mouse IGF-1 Standard with 1 ml of MIX Diluent to generate a stock solution of 10 ng/ml. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare triplicate standard points by serially diluting the Standard solution (10 ng/ml) 1:2 with equal volume of MIX Diluent to produce 5, 2.5, 1.25, 0.63, 0.32 and 0.16 ng/ml. MIX Diluent serves as the zero standard (0 ng/ml). Any remaining solution should be frozen at -20⁰C.

Standard Point	Dilution	[mIGF-1] (ng/ml)
P1	1 part Standard (10 ng/ml)	10.00
P2	1 part P1 + 1 part MIX Diluent	5.00
P3	1 part P2 + 1 part MIX Diluent	2.50
P4	1 part P3 + 1 part MIX Diluent	1.25
P5	1 part P4 + 1 part MIX Diluent	0.63
P6	1 part P5 + 1 part MIX Diluent	0.32
P7	1 part P6 + 1 part MIX Diluent	0.16
P8	MIX Diluent	0.00

- **Biotinylated IGF-1 Antibody (100x):** Spin down the antibody briefly and dilute the desired amount of the antibody 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C.
- **Wash Buffer Concentrate (20x):** Dilute the Wash Buffer Concentrate 1: 20 with reagent grade water.
- **Streptavidin-Peroxidase Conjugate (100x):** Spin down the SP Conjugate briefly and dilute the desired amount of the conjugate 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C.

Assay Procedure


- Prepare all reagents, working standards and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature (20-30°C).
- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccant inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 50 µl of Standard or sample per well, and cover wells and incubate for two hours. Start the timer after the last sample addition.
- Wash five times with 200 µl of Wash Buffer. Invert the plate and decant the contents, and blot it on absorbent paper towel to completely remove liquid at each step.
- Add 50 µl of Biotinylated IGF-1 Antibody to each well and incubate for two hours.
- Wash five times with 200 µl of Wash Buffer.
- Add 50 µl of Streptavidin-Peroxidase Conjugate per well and incubate for 30 minutes. Turn on the microplate reader and set up the program in advance.
- Wash five times with 200 µl of Wash Buffer.
- Add 50 µl of Chromogen Substrate per well and incubate for about 10 minutes or till the optimal blue color density develops. Gently tap plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50 µl of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm immediately.

Data Analysis

- Calculate the mean value of the triplicate readings for each standard and sample.
- To generate a Standard Curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis and draw a best-fit curve through the points on the graph. Plotting the log-log graph may linearize the data and the best-fit line can be determined by regression analysis of the linear portion of the curve.
- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

Standard Curve

- The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.

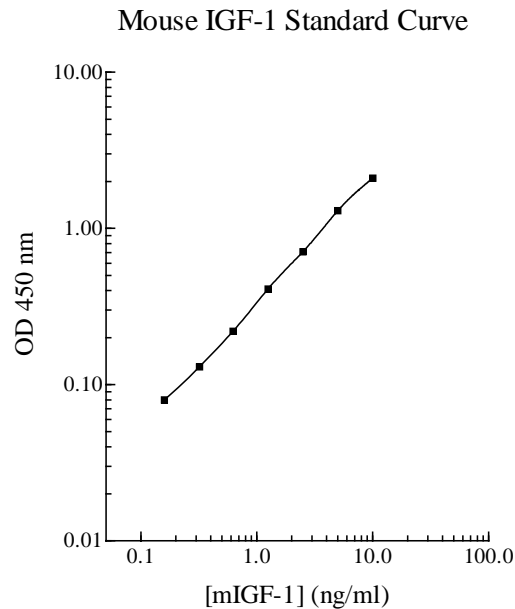

Performance Characteristics

- The minimum detectable dose of IGF-1 is typically 0.1 ng/ml.
- Intra-assay and inter-assay coefficients of variation were 4.8 % and 7.2% respectively.

Linearity

Sample Dilution	Average Percentage of Expected Value	
	Plasma	Serum
1:250	96%	100%
1:500	100%	101%
1:1000	102%	102%

Recovery

Standard Added Value	0.5 – 5 ng/ml
Recovery %	88-112 %
Average Recovery %	100 %

Cross-Reactivity

Species	% Cross Reactivity
Beagle	None
Monkey	None
Mouse	100%
Rat	100%
Swine	None

References

1. Sandberg-Nordqvist AC *et al.* (1993) *Cancer Res.* 53: 2475-2478
2. Jones JI and Clemmons DR (1995) *Endocr. Rev.* 16: 3-34
3. Moser C. *et al.* (2008) *Eur. J. Cancer* 44: 1577-1586
4. Remacle-Bonnet MM *et al.* (2000) *Cancer Res.* 60: 2007-2017
5. Adlerz L *et al.* (2007) *J. Biol. Chem.* 282: 10203 -10209
6. Sandhu MS (2005) *Endocr. Dev.* 9:44-54
7. Sima AA and Li ZG (2006) *Rev. Diabet. Stud.* 3: 161-168
8. Butovsky O *et al.* (2006) *Proc. Natl. Acad. Sci. U.S.A.* 103: 11784-11789
9. Jo H *et al.* (2008) *Mol. Cell Biol.* 28: 4285-4299
10. Spencer EM *et al.* (1991) *Bone* 12: 21-26
11. Gomez JM (2008) *Endocr. Metab. Immune Disord Drug Targes* 8: 143-151

Version 1.2