



AssayMax Mouse alpha Macroglobulin ELISA Kit (Plasma and Serum Samples)

Catalog No. EMM2115-1

Introduction

Alpha-2-Macroglobulin is a major serum protein with diverse functions, including inhibition of protease activity and binding of growth factors, cytokines, and disease factors (1). Increased serum alpha-2-Macroglobulin has been suggested to be associated with multiple sclerosis (MS) (2), glomerular disease (3), and with liver diseases (4).

Mouse alpha-Macroglobulin (M-AMG) is believed to be a functional homologue of human alpha 2-Macroglobulin (h-alpha 2M).

Principal of the Assay

The AssayMax Mouse alpha Macroglobulin ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for detection of mouse alpha Macroglobulin in plasma, and serum. This assay employs a quantitative competitive enzyme immunoassay technique that measures mouse alpha Macroglobulin in less than 3 hours. A polyclonal antibody specific for mouse alpha Macroglobulin has been pre-coated onto a 96-well microplate with removable strips. Alpha Macroglobulin in standards and samples is competed by a biotinylated alpha Macroglobulin sandwiched by the immobilized antibody and streptavidin-peroxidase conjugate. All unbound material is then washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured.

Caution and Warning

- This kit is for research use only.
- The kit should not be used beyond the expiration date.
- The Stop Solution is an acid solution.

Reagents

- **Alpha Macroglobulin Microplate:** A 96-well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody against alpha Macroglobulin.
- **Sealing Tapes:** Each kit contains 3 pre-cut, pressure-sensitive sealing tapes that can be cut to fit the format of the individual assay.
- **Alpha Macroglobulin Standard:** Mouse alpha Macroglobulin in a buffered protein base (50 µg, lyophilized).
- **Biotinylated Alpha Macroglobulin:** 1 vial, lyophilized.

- **MIX Diluent Concentrate (10x):** A 10-fold concentrated buffered protein base (30 ml).
- **Wash Buffer Concentrate (20x):** A 20-fold concentrated buffered surfactant (30 ml).
- **Streptavidin-Peroxidase Conjugate (SP Conjugate):** A 100-fold concentrate (80 μ l).
- **Chromogen Substrate:** A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution:** A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

Storage Condition

- Store kit at 2-8⁰C or -20⁰C upon arrival up to the expiration date.
- Opened MIX Diluent may be stored for up to 1 month at 2-8⁰C. Store reconstituted reagents at -20⁰C or below.
- Opened unused strip wells may return to the foil pouch with the desiccant pack, reseal along zip-seal. May be stored for up to 1 month in a vacuum desiccator.

Other Supplies Required

- Microplate reader capable of measuring absorbance at 450 nm
- Pipettes (1-20 μ l, 20-200 μ l, 200-1000 μ l and multiple channel)
- Deionized or distilled reagent grade water

Sample Collection, Preparation and Storage

- **Plasma:** Collect plasma using one-tenth volume of 0.1 M sodium citrate as an anticoagulant. Centrifuge samples at 2000 x g for 10 minutes and assay. Dilute samples 1:200 with MIX Diluent. The undiluted samples can be stored at -20⁰C or below for up to 3 months. Avoid repeated freeze-thaw cycles. (EDTA or Heparin can also be used as anticoagulant.)
- **Serum:** Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 2000 x g for 10 minutes. Remove serum and assay. Dilute samples 1:200 into MIX Diluent. The undiluted samples can be stored at -20⁰C or below for up to 3 months. Avoid repeated freeze-thaw cycles.

Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use. If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved.
- **MIX Diluent Concentrate (10x):** Dilute MIX Diluent Concentrate 1:10 with reagent grade water. Store for up to 1 month at 2-8⁰C.
- **Standard Curve:** Reconstitute the 50 μ g of Mouse alpha Macroglobulin Standard with 0.5 ml of MIX Diluent to generate a stock solution of 100 μ g/ml. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare duplicate or triplicate standard points by serially diluting the alpha Macroglobulin standard solution (100 μ g/ml) 1:2 with MIX Diluent to produce 50, 25, 12.5, 6.25, 3.13 and 1.56 μ g/ml solutions. MIX Diluent serves as the zero standard (0 μ g/ml). Any remaining solution should be frozen at -20⁰C.

Standard Point	Dilution	[Alpha Macroglobulin] ($\mu\text{g/ml}$)
P1	1 part Standard (100 $\mu\text{g/ml}$)	100.00
P2	1 part P1 + 1 part MIX Diluent	50.00
P3	1 part P2 + 1 part MIX Diluent	25.00
P4	1 part P3 + 1 part MIX Diluent	12.50
P5	1 part P4 + 1 part MIX Diluent	6.25
P6	1 part P5 + 1 part MIX Diluent	3.13
P7	1 part P6 + 1 part MIX Diluent	1.56
P8	MIX Diluent	0.00

- **Biotinylated Alpha Macroglobulin (2x):** Dilute Biotinylated alpha Macroglobulin with 4 ml MIX Diluent to produce a 2-fold stock solution. Allow the biotin to sit for 10 minutes with gentle agitation prior to making dilutions. The stock solution should be further diluted 1:2 with MIX Diluent. Any remaining solution should be frozen at -20°C .
- **Wash Buffer Concentrate (20x):** Dilute Wash Buffer Concentrate 1:20 with reagent grade water.
- **SP Conjugate (100x):** Spin down the SP Conjugate briefly and dilute the desired amount of the conjugate 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C .

Assay Procedure


- Prepare all reagents, working standards and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature ($20\text{-}30^{\circ}\text{C}$).
- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccant inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 25 μl of standard or sample per well, and immediately add 25 μl of Biotinylated alpha Macroglobulin to each well (on top of the Standard or sample) and mix gently. Cover wells with a sealing tape and incubate for two hours. Start the timer after the last sample addition.
- Wash five times with 200 μl of Wash Buffer manually. Invert the plate each time and decant the contents; hit it 4-5 times on absorbent paper towel to completely remove the liquid. If using a machine wash six times with 300 μl of Wash Buffer and then invert the plate, decant the contents; hit it 4-5 times on absorbent paper towel to completely remove the liquid.
- Add 50 μl of Streptavidin-Peroxidase Conjugate to each well and incubate for 30 minutes. Turn on the microplate reader and set up the program in advance.
- Wash a microplate as described above.
- Add 50 μl of Chromogen Substrate per well and incubate for about 10 minutes or until the optimal blue color density develops. Gently tap plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50 μl of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm **immediately**. If wavelength correction is available, subtract readings at 570 nm from those at 450 nm to correct optical imperfections. Otherwise, read the plate at 450 nm only. Please note that some unstable black particles may be generated at high concentration points after stopping the reaction for about 10 minutes, which will reduce the readings.

Data Analysis

- Calculate the mean value of the duplicate or triplicate readings for each standard and sample.
- To generate a standard curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis using log-log or four-parameter logistic curve-fit.
- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

Standard Curve

- The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.

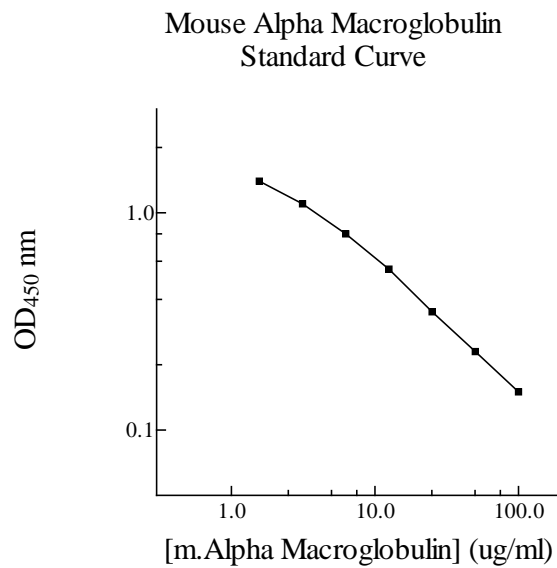

Performance Characteristics

- The minimum detectable level of alpha Macroglobulin is typically < 1 µg/ml.
- Intra-assay and inter-assay coefficients of variation were 5.0 % and 7.1% respectively.

Linearity

Sample Dilution	Average Percentage of Expected Value	
	Plasma	Serum
1:100	98%	97%
1:200	100%	101%
1:400	106%	107%

Recovery

Standard Added Value	4 – 40 ug/ml
Recovery %	80-110 %
Average Recovery %	95 %

Cross-Reactivity

Species	% Cross Reactivity
Beagle	None
Monkey	None
Human	None
Rat	< 10 (suggest 1:20 dilution for Plasma/Serum samples)
Swine	< 1
Rabbit	None

Reference Value

- The average mouse blood levels of alpha Macroglobulin is 1.5 g/L.

References

- (1) Pineda-Salgado L *et al* (2005) *Gene Expr Patterns*. 6(1):3-10
- (2) Jensen PE *et al* (2004) *Biochim Biophys Acta*. 5:1690(3):203-7
- (3) Yang AH *et al* (1997) *Nephrol Dial Transplant*. 12(3):465-9
- (4) Shiota G *et al* (1995) *J Med*. 26(5-6):295-308

Version 1.2R

Related Products

- EM1115-1 AssayMax Human alpha-2-Macroglobulin ELISA Kit (Saliva, Milk and Cell Culture Supernatant samples)
- EM2115-1 AssayMax Human alpha-2-Macroglobulin ELISA Kit (Plasma and Serum samples)
- EMM1115-1 AssayMax Mouse alpha Macroglobulin ELISA Kit (Cell Culture Supernatant samples)