



AssayMax Rat Ceruloplasmin ELISA Kit (Plasma and Serum Samples)

Catalog Number ERC4001-1

Introduction

Ceruloplasmin is an abundant α_2 -serum glycoprotein that contains 95% of the copper found in the plasma of vertebrate species (1). Ceruloplasmin is a copper-binding protein that normally removes iron from cells by its ferroxidase activity. Ceruloplasmin concentration on average is 14.6 (± 4.0) mg/dl (2). Low levels of ceruloplasmin lead to the abnormal deposition of iron in cells, including those of the pancreas, liver, retina and the basal ganglia region of the brain. Some diseases associated with ceruloplasmin are Wilson's disease (3), Hemochromatosis (4), Menkes disease (5) and Aceroluplasminemia (1).

Principal of the Assay

The AssayMax Rat Ceruloplasmin ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for detection of rat ceruloplasmin in plasma, and serum. This assay employs a quantitative competitive enzyme immunoassay technique that measures rat ceruloplasmin in less than 3 hours. A polyclonal antibody specific for rat ceruloplasmin has been pre-coated onto a 96-well microplate with removable strips. Ceruloplasmin in standards and samples is competed by a biotinylated ceruloplasmin sandwiched by the immobilized antibody and streptavidin-peroxidase conjugate. All unbound material is then washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured.

Caution and Warning

- This kit is for research use only.
- The kit should not be used beyond the expiration date.
- The Stop Solution is an acid solution.

Reagents

- **Rat Ceruloplasmin Microplate:** A 96-well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody against rat Ceruloplasmin.
- **Sealing Tapes:** Each kit contains 3 pre-cut, pressure-sensitive sealing tapes that can be cut to fit the format of the individual assay.
- **Rat Ceruloplasmin Standard:** Rat Ceruloplasmin in a buffered protein base (25 μ g, lyophilized).
- **Biotinylated Ceruloplasmin:** 1 vial, lyophilized.
- **MIX Diluent Concentrate (10x):** A 10-fold concentrated buffered protein base (30 ml).

- **Wash Buffer Concentrate (20x):** A 20-fold concentrated buffered surfactant (30 ml).
- **Streptavidin-Peroxidase Conjugate (SP Conjugate):** A 100-fold concentrate (90 μ l).
- **Chromogen Substrate:** A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution:** A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

Storage Condition

- Store kit at 2-8⁰C or -20⁰C upon arrival up to the expiration date.
- Opened MIX Diluent may be stored for up to 1 month at 2-8⁰C. Store reconstituted reagents at -20⁰C or below.
- Opened unused strip wells may return to the foil pouch with the desiccant pack, reseal along zip-seal. May be stored for up to 1 month in a vacuum desiccator.

Other Supplies Required

- Microplate reader capable of measuring absorbance at 450 nm.
- Pipettes (1-20 μ l, 20-200 μ l, 200-1000 μ l and multiple channel).
- Deionized or distilled reagent grade water.

Sample Collection, Preparation and Storage

- **Plasma:** Collect plasma using one-tenth volume of 0.1 M sodium citrate as an anticoagulant. Centrifuge samples at 2000 x g for 10 minutes and assay. Dilute samples 1:400 into MIX Diluent. The undiluted samples can be stored at -20⁰C or below for up to 3 months. Avoid repeated freeze-thaw cycles. (EDTA or Heparin can also be used as anticoagulant.)
- **Serum:** Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 2000 x g for 10 minutes. Remove serum and assay. Dilute samples 1:400 into MIX Diluent. The undiluted samples can be stored at -20⁰C or below for up to 3 months. Avoid repeated freeze-thaw cycles.

Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use. If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved.
- **MIX Diluent Concentrate (10x):** Dilute the MIX Diluent 1:10 with reagent grade water. Store for up to 1 month at 2-8⁰C.
- **Standard Curve:** Reconstitute the 25 μ g of Ceruloplasmin Standard with 0.5 ml of MIX Diluent to generate a solution of 50 μ g/ml. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare triplicate standard points by serially diluting the standard solution (50 μ g/ml) 1:2 with MIX Diluent to produce 25, 12.5, 6.25, 3.13, 1.56 and 0.78 μ g/ml solutions. MIX Diluent serves as the zero standard (0 μ g/ml). Any remaining solution should be frozen at -20⁰C.

Standard Point	Dilution	[Ceruloplasmin] ($\mu\text{g/ml}$)
P1	Standard (50 $\mu\text{g/ml}$)	50.00
P2	1 part P1 + 1 parts MIX Diluent	25.00
P3	1 part P2 + 1 parts MIX Diluent	12.50
P4	1 part P3 + 1 parts MIX Diluent	6.25
P5	1 part P4 + 1 parts MIX Diluent	3.13
P6	1 part P5 + 1 parts MIX Diluent	1.56
P7	1 part P6 + 1 parts MIX Diluent	0.78
P8	MIX Diluent	0.00

- **Biotinylated Ceruloplasmin (2x):** Dilute Biotinylated Ceruloplasmin with 4 ml MIX Diluent to produce a 2-fold solution. Allow the biotin to sit for 10 minutes with gentle agitation prior to making dilutions. The stock solution should be further diluted 1:2 with MIX Diluent. Any remaining solution should be frozen at -20°C .
- **Wash Buffer Concentrate (20x):** Dilute the Wash Buffer Concentrate 1:20 with reagent grade water.
- **SP Conjugate (100x):** Spin down the SP Conjugate briefly and dilute the desired amount of the conjugate 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C .

Assay Procedure

- Prepare all reagents, working standards and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature ($20\text{-}30^{\circ}\text{C}$).
- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccant inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 25 μl of standard or sample per well, and immediately add 25 μl of Biotinylated Ceruloplasmin to each well (on top of the Standard or sample) and mix gently. Cover wells with a sealing tape and incubate for two hours. Start the timer after the last sample addition.
- Wash five times with 200 μl of Wash Buffer. Invert the plate and decant the contents, and hit it 4-5 times on absorbent paper towel to complete remove liquid at each step.
- Add 50 μl of Streptavidin-Peroxidase Conjugate to each well and incubate for 30 minutes. Turn on the microplate reader and set up the program in advance.
- Wash five times with 200 μl of Wash Buffer.
- Add 50 μl of Chromogen Substrate per well and incubate for about 10 minutes or till the optimal blue color density develops. Gently tap plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50 μl of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm **immediately**. Please note that after the reaction is stopped for about 10 minutes, some black particles may be generated at high concentration point, which will reduce the readings.


Data Analysis

- Calculate the mean value of the triplicate readings for each standard and sample. To generate a Standard Curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis using log-log or four-parameter logistic curve-fit.

- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

Standard Curve

- The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.

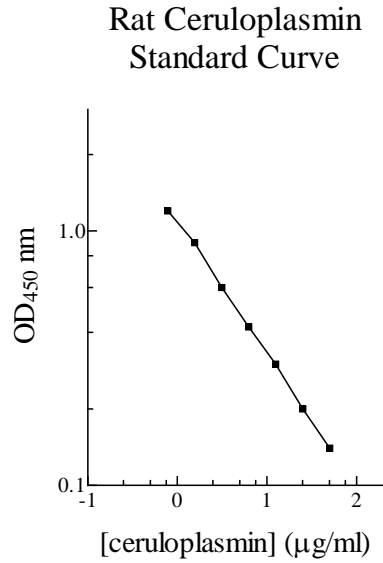

Precision, Sensitivity and Specificity

- The minimum detectable dose of Ceruloplasmin is typically 500 ng/ml.
- Intra-assay and inter-assay coefficients of variation were 4.4% and 7.0% respectively.

Linearity

Sample Dilution	Plasma	Serum
1:50	92%	96%
1:100	107%	103%
1:200	110%	111%

Recovery

Standard Added Value	1 – 20 µg/ml
Recovery %	80-110 %
Average Recovery %	95 %

Cross-Reactivity

Species	% Cross Reactivity
Beagle	None
Bovine	None
Monkey	None
Mouse	< 5
Human	None
Swine	< 2

Reference Value: Average rat plasma ceruloplasmin concentration is 300 µg/ml.

References

- (1) Harris, Z. L, et al. *Proc. Natl. Acad. Sci.* Vol. 92, pp. 2539-2543, March 1995
- (2) Aliyazicioğlu, Y et al. *The Turkish Journal of Pediatrics* 2007; 49: 52-54
- (3) Czaja, M. J et al. *J. Clin. Invest.* Volume 80, October 1987, 1200-1204
- (4) Kumar, A et al. *WJM, October 1995-Vol 163, No. 4*
- (5) Moller, L.B. et al. *Am. J. Hum. Genet.* 66:1211–1220, 2000

Version 1.1

Related Products

- EC4101-1 AssayMax Human Ceruloplasmin ELISA Kit (Urine & Cell Culture Samples)
- EC4001-1 AssayMax Human Ceruloplasmin ELISA Kit (Plasma & Serum Samples)
- ERC4101-1 AssayMax Rat Ceruloplasmin ELISA Kit (Urine & Cell Culture Samples)